

ANALYSIS CERTIFICATE

Manufacturer Name and Address: Thermo Fisher Scientific Oy
Ratastie 2, FIN-01620 Vantaa, Finland

Product Name : Magnesium

Catalogue no. : 981385

Lot no. : E129

Package : 12 x 20 ml

Storage Conditions : 2...25 °C


Expiry date : 2011-02

**Quality Control
Performance test:**

<u>Control (lot)</u>	<u>Result (mmol/l)</u>	<u>Target range (mmol/l)</u>
Abtrol (D390)	1,30	1,18 - 1,38
Nortrol (D389)	0,81	0,73 - 0,85

This product with the mentioned lot number was analysed by our authorised quality control department and confirmed that it meets its specifications.

Vantaa 18 / 3 2009


Hannele Laine
Quality Assurance Specialist
Quality Regulatory and Compliance
Clinical Diagnostics Finland

18/03/2009 07:50

981385 E 129 2011-02


Test MG

Accepted 18/03/2009 07:01

Factor 4.555
 Bias -0.006

Coeff. of det. 0.999993

Errors

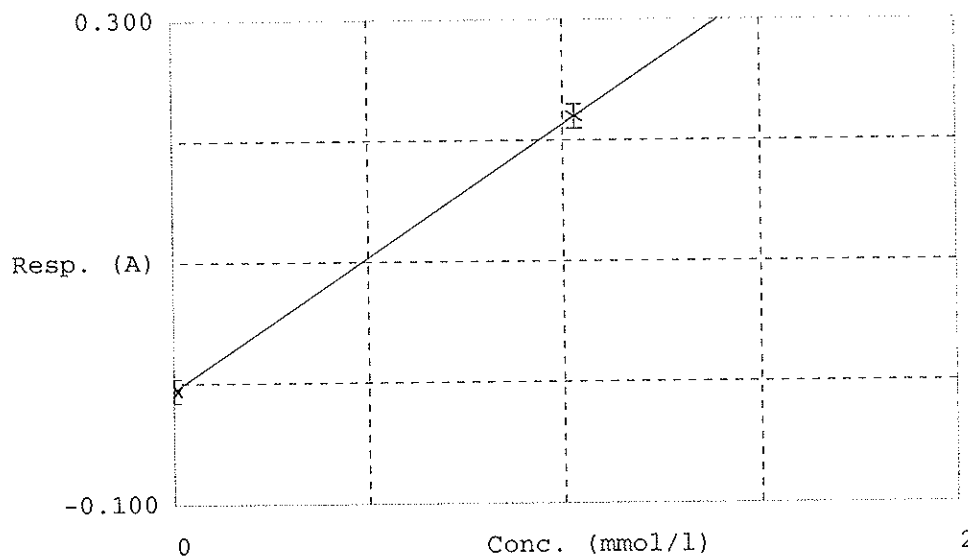

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Water	-0.006	0.002	0.000	
2	Water	-0.007	-0.002	0.000	
3	sCal	0.220	1.030	1.030	
4	sCal	0.220	1.030	1.030	
5	Nortrol(control)	0.170	0.805	0.790	
6	Abtrol(control)	0.278	1.295	1.280	